


BA 400
LED TECHNOLOGY

Smart Efficiency
Biochemistry Analyzer

BioSystems
REAGENTS & INSTRUMENTS

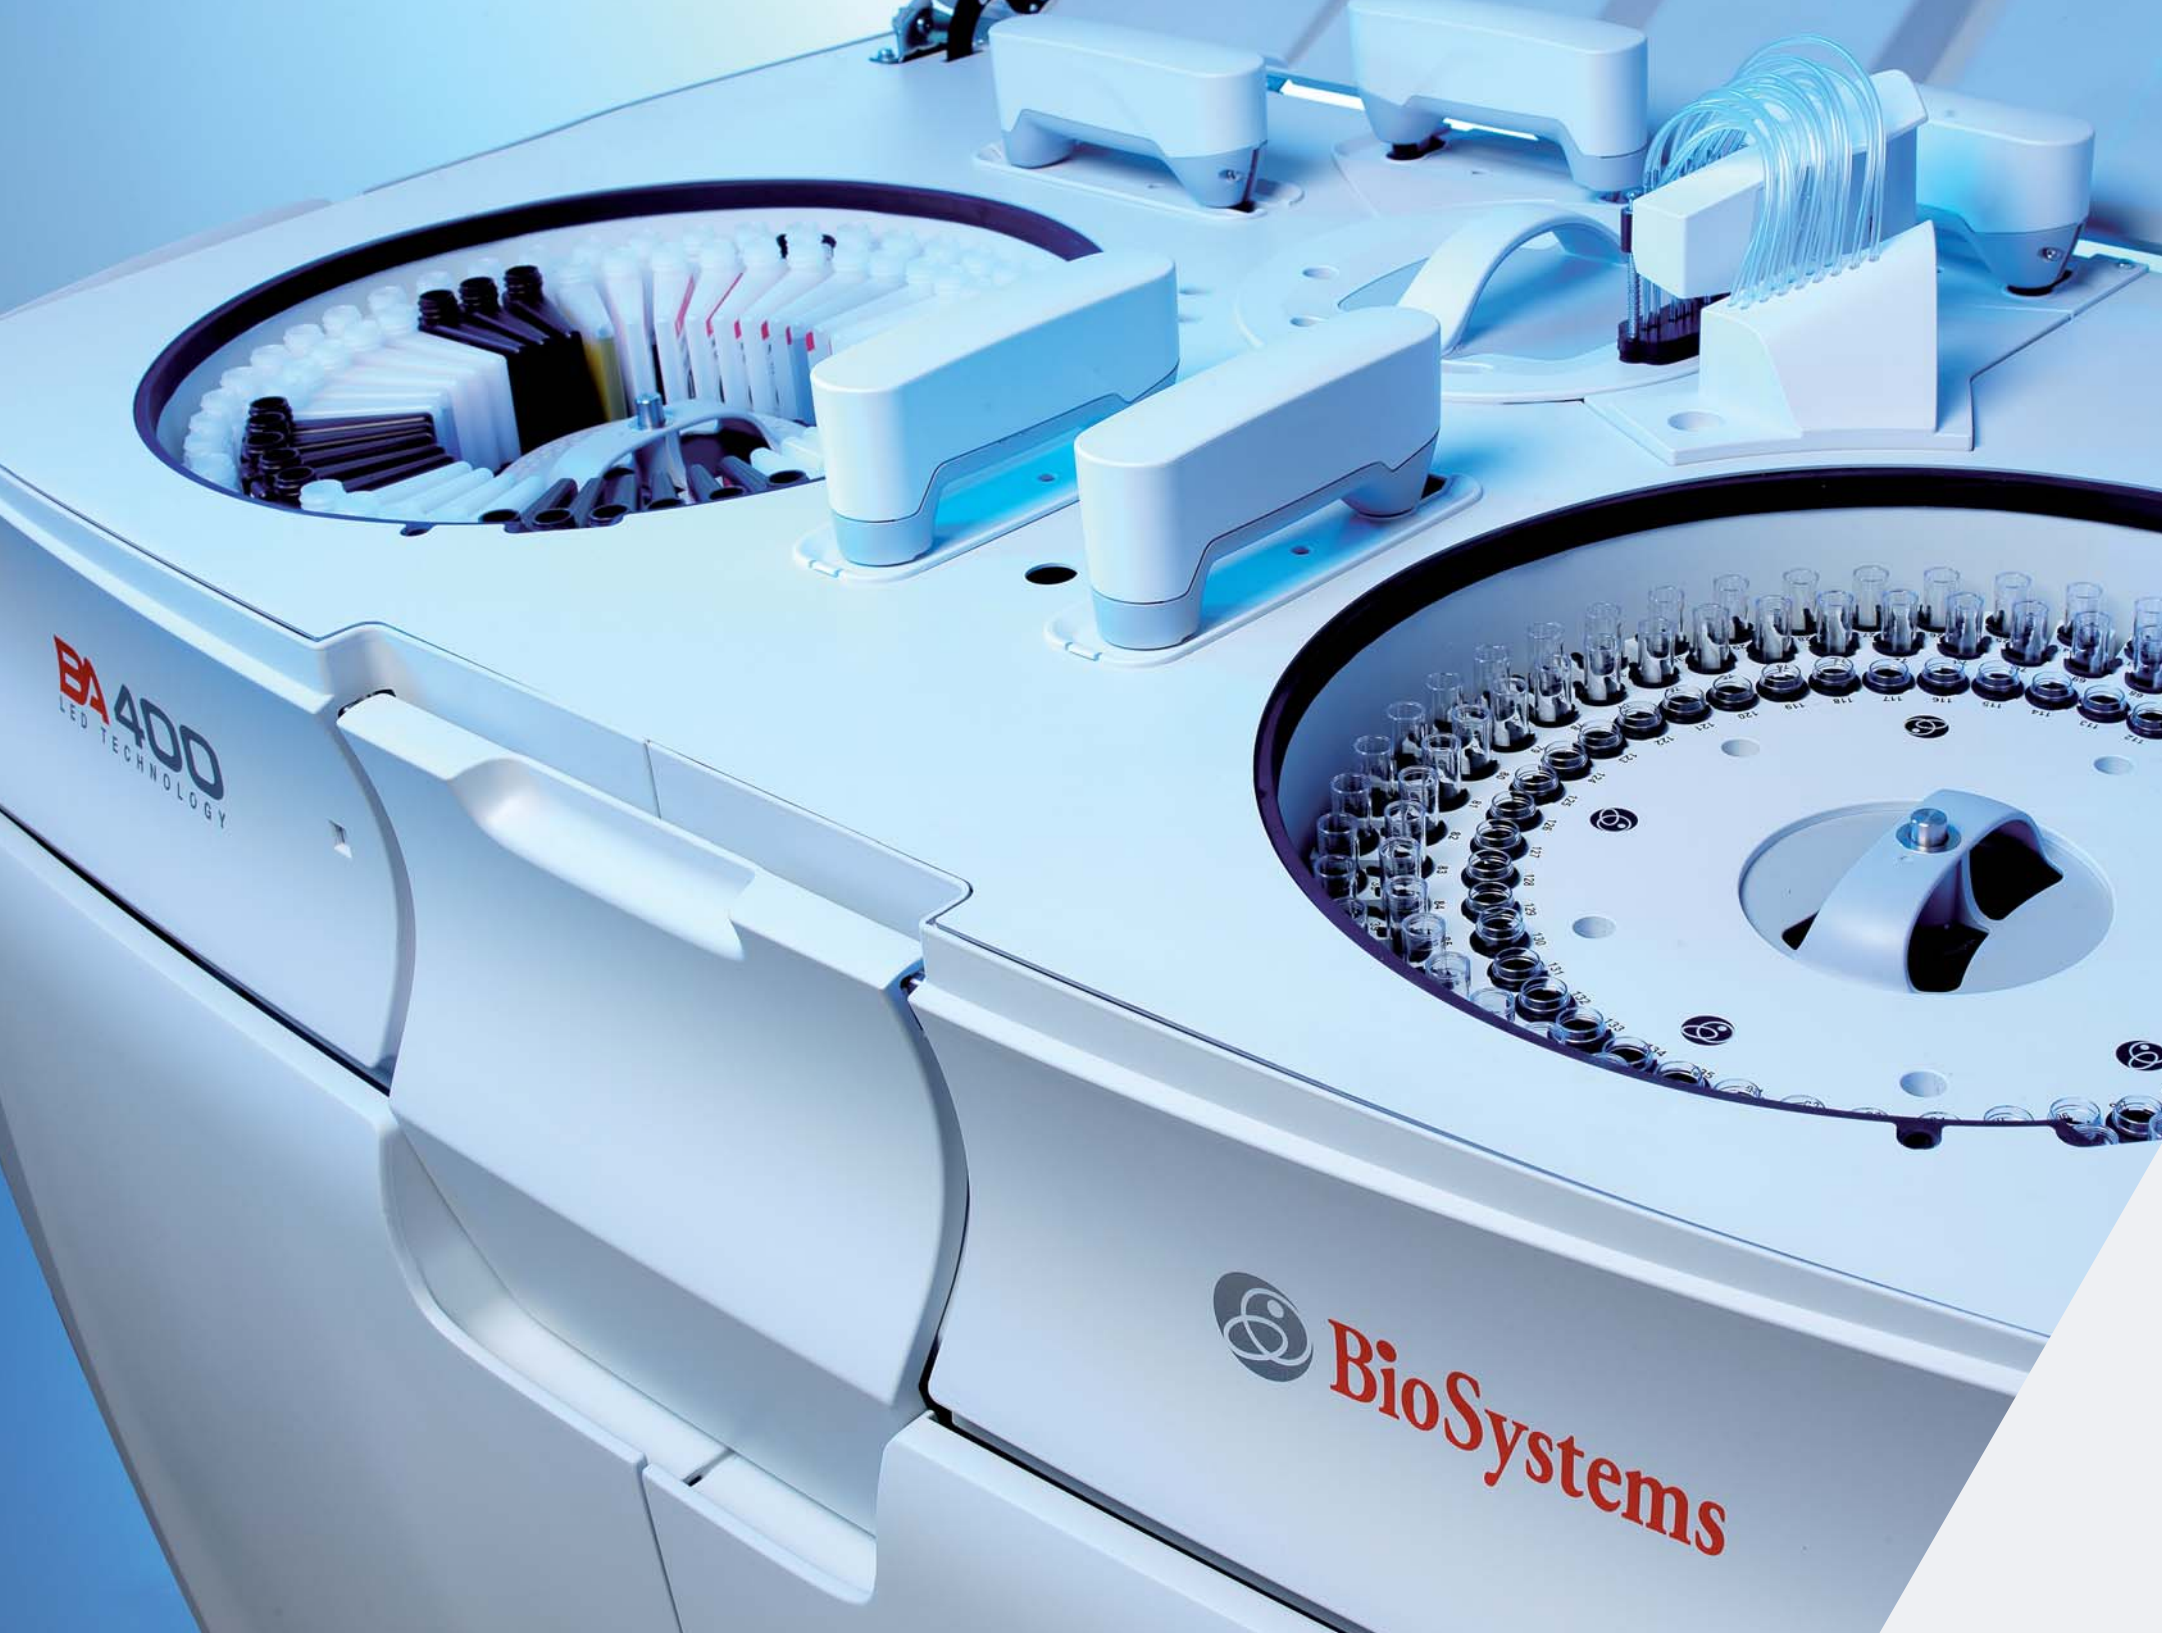

BA400
LED TECHNOLOGY

 **BioSystems**




Smart Efficiency

BioSystems designs and develops efficient systems that implement the latest and best technical solutions.

BioSystems' BA400 is a clinical chemistry and turbidimetry analyzer designed to offer the best performance to laboratories looking towards achieving highest efficiency with optimal operative cost.

In combination with BioSystems original reagents and worldwide technical support coverage, the BA400 system defines the new generation of clinical analyzers.

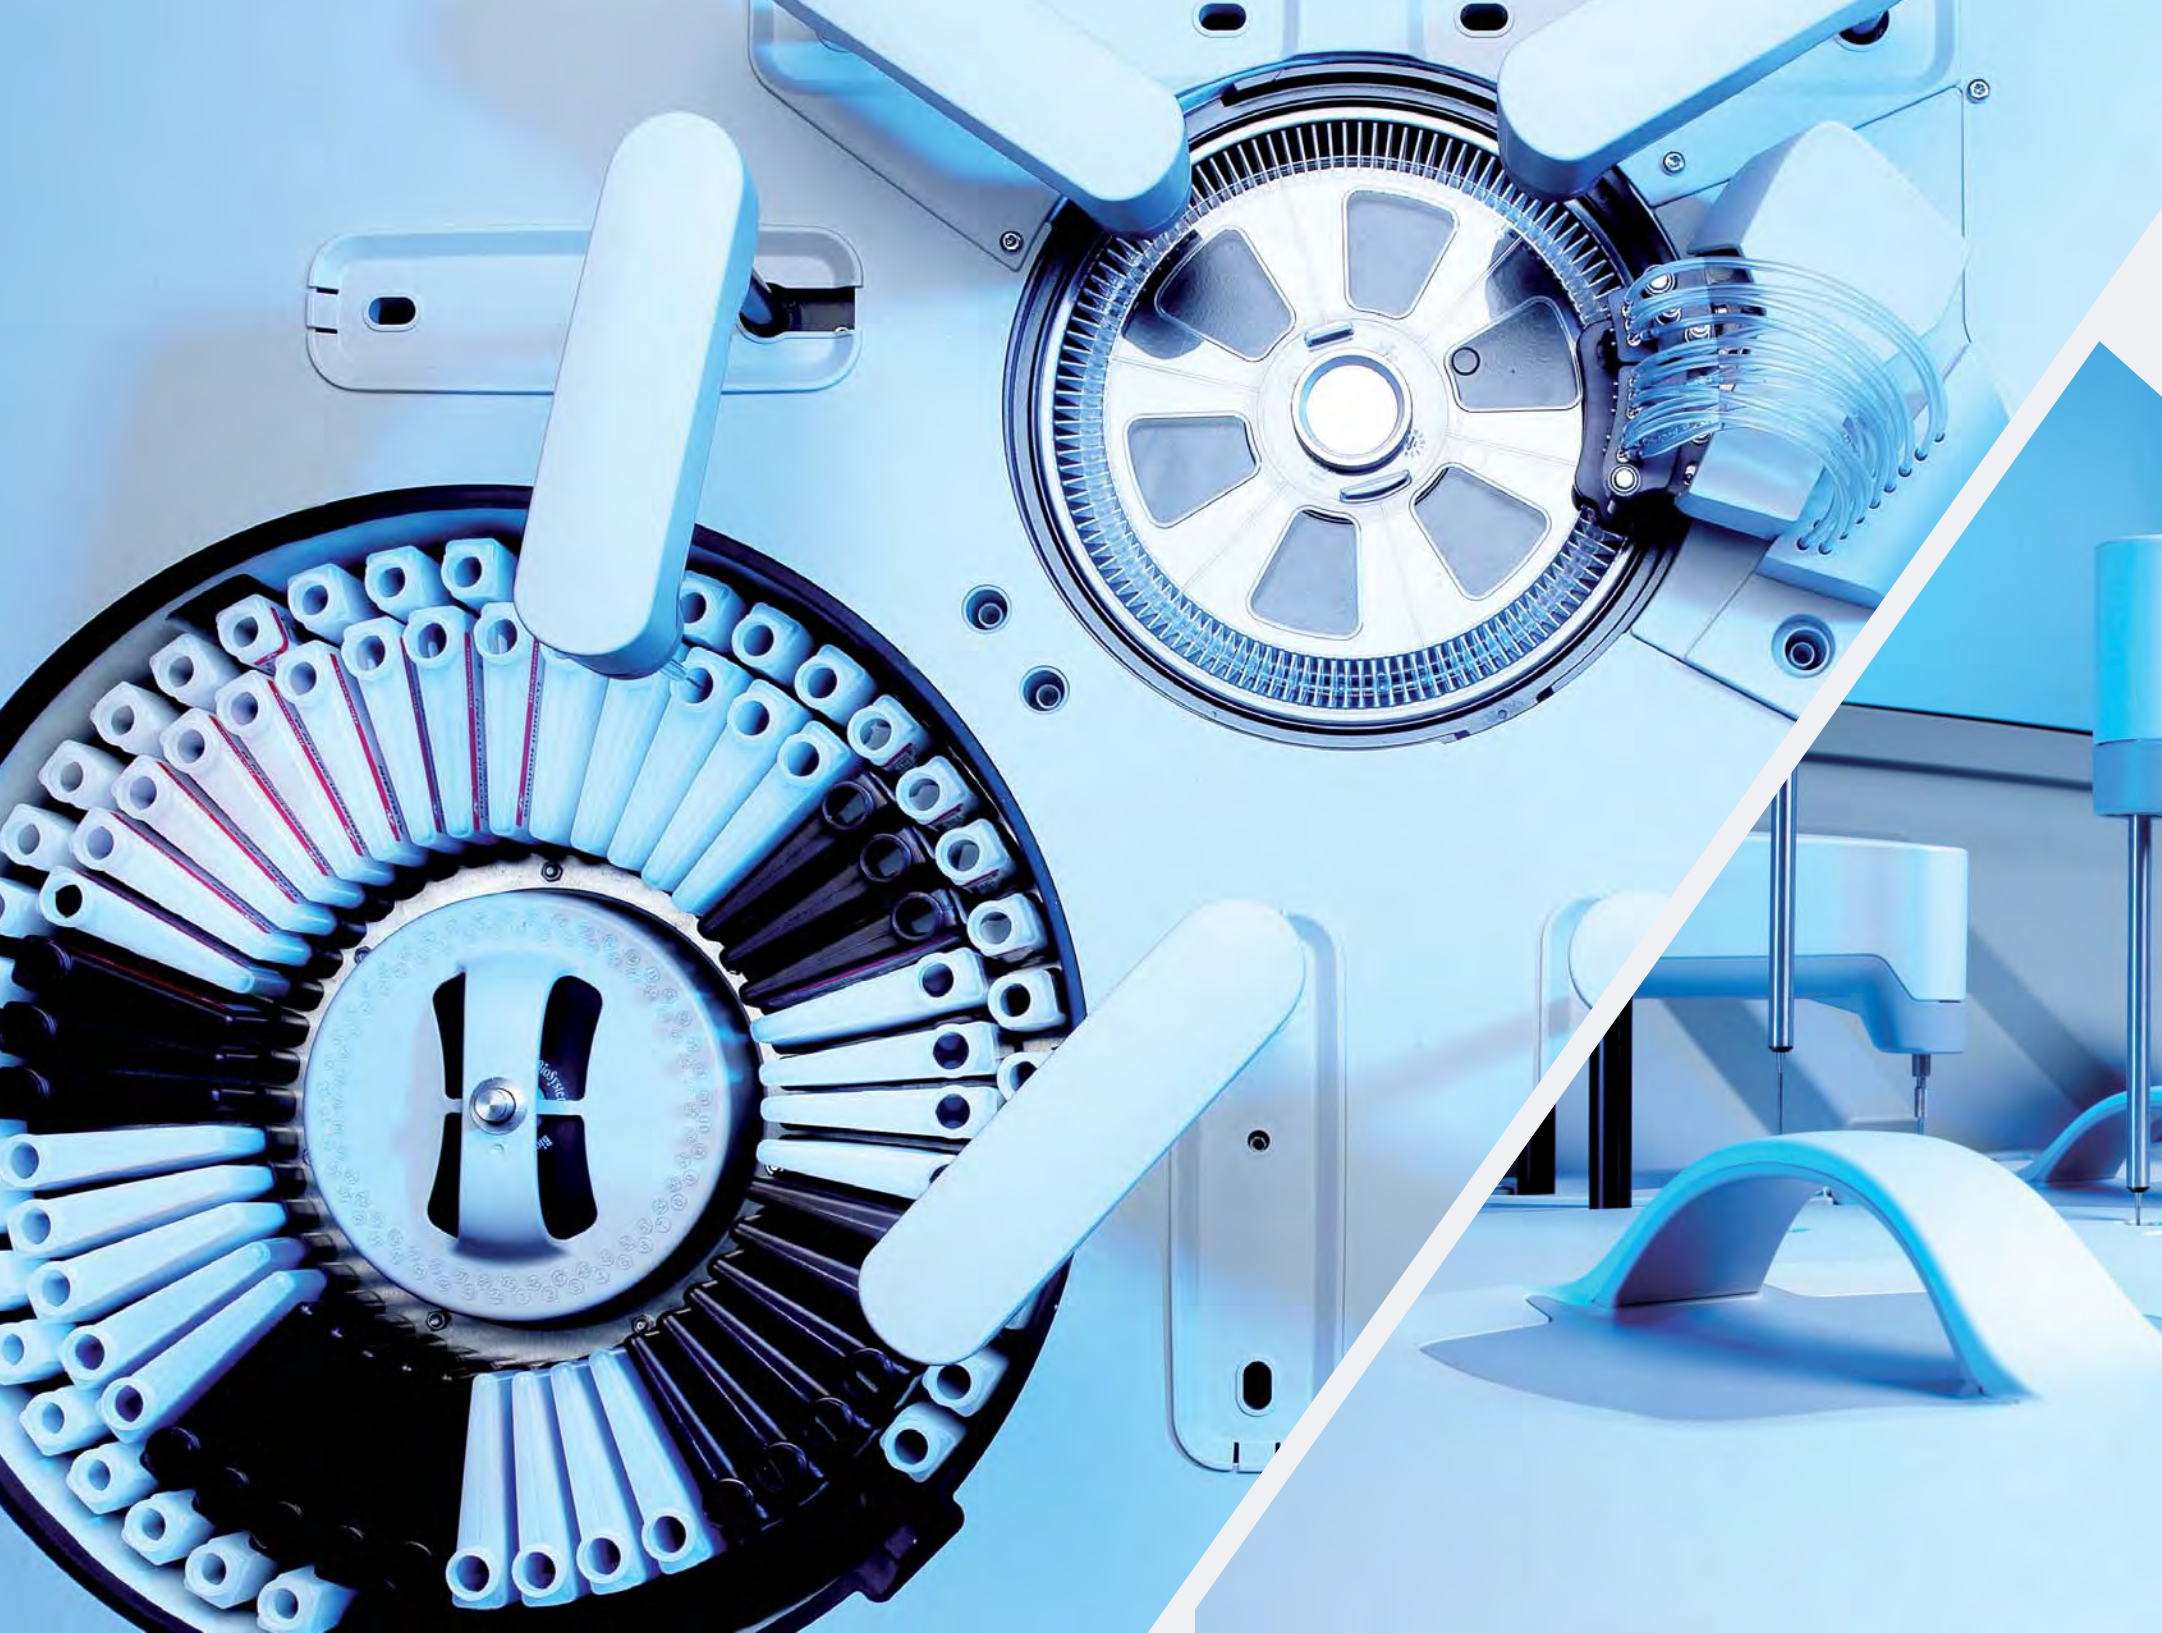

Smart Autonomy

88 refrigerated positions with internal barcode reader.

135 positions for samples, controls and standards suitable for primary or paediatric tubes, 90 of them with barcode reading.

High capacity washing solution and waste containers, able to operate up to 8 hours of continuous working without refilling/voiding.

Automated water inlet and waste outlet with internal reservoirs, easy to adapt to any lab facilities.

Smart Optics

BioSystems has developed for its BA400 analyzer an advanced and innovative optical system based on a battery of high power LED monochromatic sources with 8 working wavelengths that covers the most demanding methods of routine and special chemistry.

Solid-state light source with a split reference beam, with a working life up to 50.000 hours, to achieve optimal accuracy and performance.

Smart Performance

Self-controlled electronic subsystems through CAN bus optimize performance and reduce maintenance down-times.

Sample dispensing system of high accuracy with level, collision and clot detection that automatically retreats to a protected home position during stops.

Low water consumption (less than 14 L/hour) with thermostated fluid washing station system to keep rotor temperature stable.

Low mechanical wear dispensing pumps with ceramic piston.

Independent powered cooling system for reagents (temperature between 5 and 8 °C, up to 35 °C room temperature).





Smart Solutions



High operating autonomy, through its high capacity for samples and reagents.

Optical system with BioSystems' patented LED technology, with virtually no maintenance.

Low operating cost with optimized water and power consumption, minimum reaction volume and high pipetting precision.

Distributed electronics through CAN (Controller Area Network) bus system to increase robustness, simplify maintenance and reduce down times.

User friendly software, with intuitive graphical interface, real time monitoring of work-session and exhaustive quality control analysis (Westgard rules, Youden and Levy-Jennings charts, historical results database management).

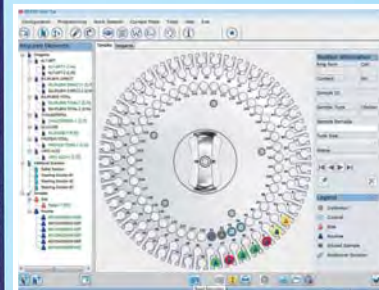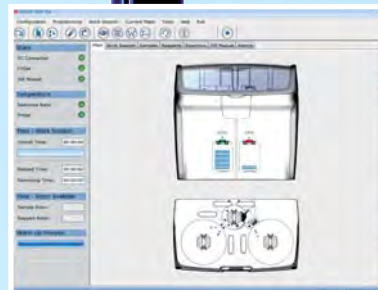

Smart System

Original reagents specially designed and optimized for its use in the BA400 system, covering a complete panel of clinical chemistry and specific protein tests.

Worldwide technical assistance coverage with BioSystems' certified engineers.

BioSystems SA, as a European manufacturer of its own reagents and analyzers, ensures proper functionality of all components under strict quality and safety standards for maximum performance and capabilities of their systems.

Turbidimetry

Code	Test	Presentation		
		R1	R2	mL/Kit
22324	Albumin (Microalbuminuria)	4x60 mL	4x15 mL	300
22923	Anti-Streptolysin O (ASO)	2x60 mL	2x15 mL	150
22936	Antithrombin III	2x60 mL	2x15 mL	150
22928	α -1-Acid Glycoprotein	2x60 mL		120
22941	α -1-Microglobulin	2x60 mL	2x15 mL	150
22095	Apolipoprotein A-I (APO A-I)	2x60 mL	2x15 mL	150
22098	Apolipoprotein B (APO B)	2x60 mL	2x15 mL	150
22925	β 2-Microglobulin	2x60 mL	2x15 mL	150
22084	Complement Component C3	2x60 mL		120
22085	Complement Component C4	2x60 mL		120
22921	C-Reactive Protein (CRP)	4x60 mL	4x15 mL	300
22927	C-Reactive Protein-hs (CRP-hs)	2x60 mL	2x15 mL	150
22934	Ferritin	2x40 mL	2x20 mL	120
22804	Fibrinogen	2x60 mL	2x15 mL	160
22044	Hemoglobin A1C-Turbi (Hb A1C-Turbi)	1x60 mL	1x15 mL	75
22082	Immunoglobulin A (Ig A)	2x60 mL		120
22081	Immunoglobulin G (Ig G)	2x60 mL		120
22083	Immunoglobulin M (Ig M)	2x60 mL		120
22929	Prealbumin	2x60 mL		120
22922	Rheumatoid Factors (RF)	4x60 mL	4x15 mL	300
22091	Transferrin	2x60 mL		120

Biochemistry

Code	Test	Presentation		
		R1	R2	mL/Kit
21550	α -Amylase-Direct	8x20 mL		160
21534	α -Amylase-EPS	2x60 mL	2x15 mL	150
21799	α -Amylase Pancreatic	2x60 mL	2x15 mL	150
21533	Alanine Aminotransferase (ALT/GPT)	8x60 mL	8x15 mL	600
21547	Albumin	10x60 mL		600
21592	Alkaline Phosphatase (ALP)-AMP	4x60 mL	4x15 mL	300
21590	Alkaline Phosphatase (ALP)-DEA	4x60 mL	4x15 mL	300
21531	Aspartate Aminotransferase (AST/GOT)	8x60 mL	8x15 mL	600
21798	Bilirubin (Direct)	4x60 mL	3x20 mL	300
21510	Bilirubin (Total)	8x60 mL	8x15 mL	600
21570	Calcium-Arsenazo	10x60 mL		600
21570	Calcium-Cresolphthalein	8x60 mL	8x15 mL	600
21558	Carbon Dioxide (CO ₂)	2x60 mL		120
21505	Cholesterol	10x60 mL		600
21557	Cholesterol HDL Direct	2x60 mL	2x20 mL	160
21585	Cholesterol LDL Direct	2x60 mL	2x20 mL	160
21588	Cholinesterase (CHE)	2x60 mL	2x15 mL	150
21790	Creatine Kinase (CK)	2x60 mL	2x15 mL	150
21792	Creatine Kinase-MB (CK-MB)	2x60 mL	2x15 mL	150
21502	Creatinine	5x60 mL	5x60 mL	600
21520	γ -Glutamyltransferase (γ -GT)	4x60 mL	4x15 mL	300
21503	Glucose	10x60 mL		600
21509	Iron-Ferrozine	4x60 mL	4x15 mL	300
21580	Lactate Dehydrogenase (LDH)	8x60 mL	8x15 mL	600
21586	Lactate Dehydrogenase (LDH)-IFCC	8x60 mL	8x15 mL	600
21793	Lipase	2x50 mL	1x20 mL	120
21797	Magnesium	2x60 mL	2x15 mL	150
21508	Phosphorus	4x60 mL	2x50 mL	340
21500	Protein (Total)	10x60 mL		600
21501	Protein (Urine+CSF)	4x60 mL		240
21551	Total Bile Acids	2x60 mL	2x20 mL	160
21528	Triglycerides	10x60 mL		600
21516	Urea/BUN-UV	8x60 mL	8x15 mL	600
21521	Uric Acid	10x60 mL		600





CE

Technical Specifications

Throughput	400 test/h (without electrolytes)	Optical System	
Throughput ISE module	320 test/h	Light Source	LED + Hard Coating filter
Principles of analysis	Colorimetry, turbidimetry.	Wavelengths	340 - 405 - 505 - 535 - 560 - 600 - 635 - 670 nm
ISE Module (optional)		Filters bandwidth	10 nm \pm 2 nm
Sample type	Serum, Plasma or Urine	Photometric range	-0.2 A to 3.5 A
Electrode type	Na+, K+, Cl-, Li+ (optional)	Internal resolution	0.0001
Sample volume	Serum: 100 μ L / Urine: 200 μ L	Detector	Main Photodiode + reference photodiode
Sample handling		Measurement precision	CV < 1% to 0.1 A
Capacity of sample rotor	135	(for 340 nm, 405 nm and 505 nm)	CV < 0.1% to 2 A
Barcode Detector	Yes	Environmental Requirements	
Number of samples with barcode	90	Ambient temperature	From 10 °C to 35 °C
Sample tube size	Diameter from 12 mm to 16 mm (height up to 100 mm)	Relative humidity	From 10 °C to 30 °C (With ISE module)
Pediatric well	13.5 mm diameter	Altitude	< 85% without condensation
Type of syringe	Ceramic piston pump with low maintenance		< 2 500 m
Pipetting volume	from 2 μ L to 40 μ L	Dimensions and weight	
Pipetting resolution	0.1 μ L	Dimensions (width, depth and height)	1 200 mm x 720 mm x 1 258 mm
Predilution ratio	From 1:2 to 1:200	Weight	210 Kg
Level detection	Yes	Electrical Requirements	
Clot detector	Yes	Mains voltage	115 V to 230 V
Vertical collision detector	Yes	Mains frequency	50 Hz or 60 Hz
		Electric power	500 VA
Reagent handling		Fluidic Requirements	
Volume of reagent bottles	20 mL, 60 mL	Water inlet	External tank or mains water supply
Capacity of reagent rotor	88 (44 bottles of 20 mL or 60 mL + 44 bottles of 20 mL)	Water Type	Purified Type II
Cooled reagent	Yes	Water consumption	< 14 L/h
Temperature range of refrigerator	From 5 °C to 8 °C (at room temperature of 25 °C)	Internal bottle of high concentration waste	5 L
Barcode Detector	Yes	Internal bottle of washing solution	5 L
Reagent volume R1	From 150 μ L to 450 μ L	Minimum Computer Requirements	
Reagent volume R2	From 40 μ L to 300 μ L	Operating system	Windows® 7 64 bit (x64)
Type of syringe	Ceramic piston pump with low-maintenance	CPU	Equivalent to Intel Core i3 @3.10 GHz or higher
Pipetting resolution	1 μ L	RAM	4 Gbytes
Level Detection	Yes	Hard Disk	40 GB or higher
Vertical collision detector	Yes	DVD	Yes
Thermostated tip	Yes	Monitor minimum resolution	Minimum resolution 1 024 x 768
		Connector of serial channel	USB
Reactions rotor		Directives and Standards Compliance	
Minimum reaction volume	200 μ L	EC Directive	98/79/EC IVD
Maximum reaction volume	600 μ L		
Number of wells	120		
Well material	UV methacrylate		
Temperature reaction rotor	37 °C		
Accuracy of temperature	\pm 0.2 °C		
Temperature stability	\pm 0.1 °C		
Mixers	2		
Cuvette washing system	7 tips (2 wash, 3 rinse, 2 dry)		

BioSystems, S.A. reserves the right to change specifications of the instruments at any time due to technical improvements.



Ginger Group



BioSystems



- Certified Management System
- EN ISO 9001
- EN ISO 13485

Manufactured by: BioSystems S.A.

Costa Brava 30, 08030 Barcelona (Spain) Tel. +34-93 311 00 00
biosystems@biosystems.es • www.biosystems.es